

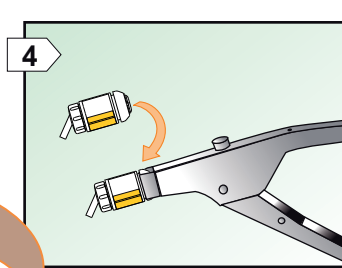
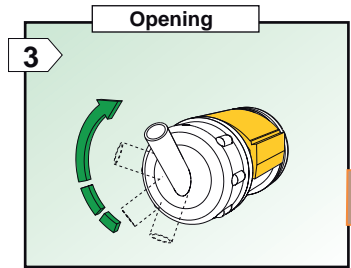
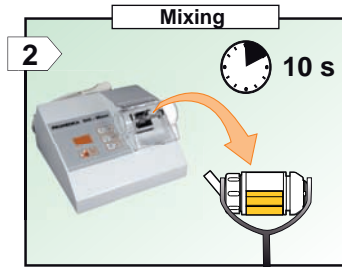
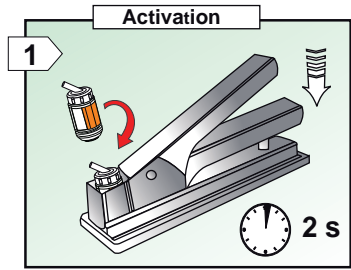
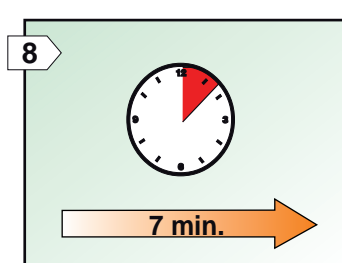
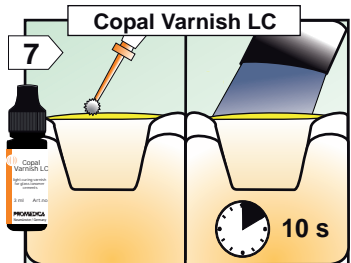


Medifil IX / Medifil IX silver AC

Instruction


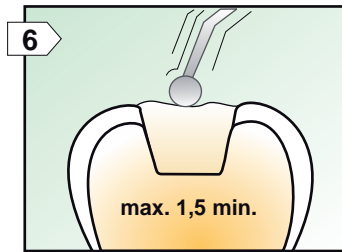


a. Filling






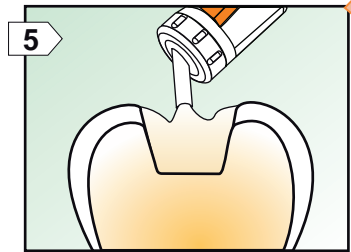


Medifil IX / Medifil IX silver AC

Instruction

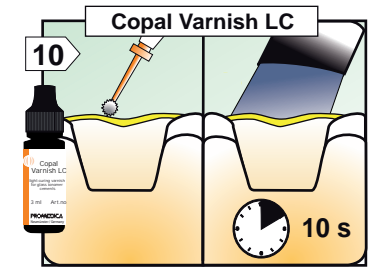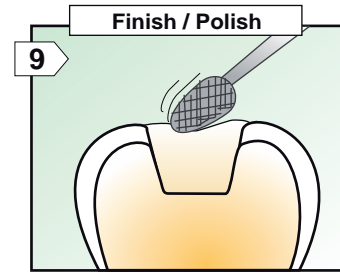

b. Core build-up

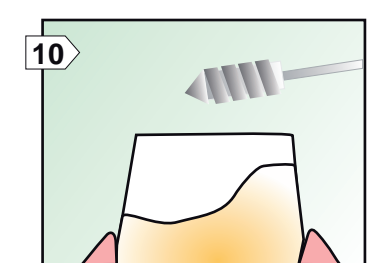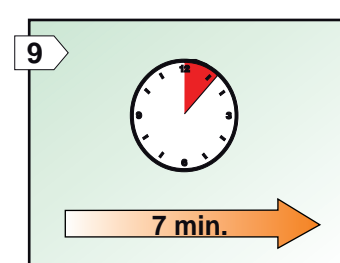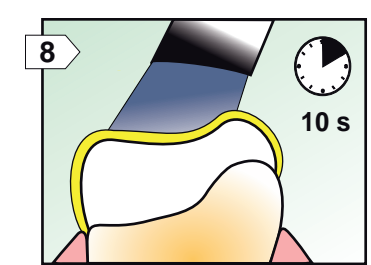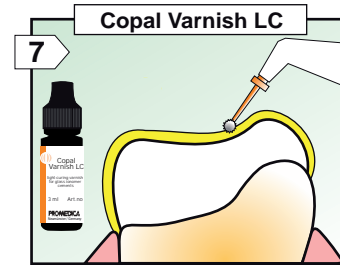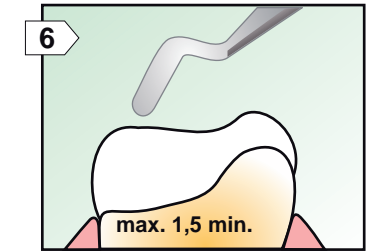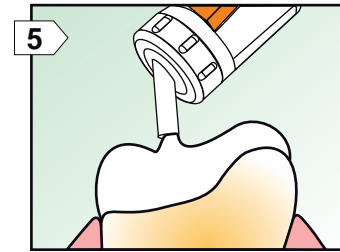

Please follow detailed instructions for use.

PROMEDICA
Dental Material GmbH
Domagkstraße 31
24537 Neumünster
Germany

PM 62002627 E1 0413 99